

# Allergen Shield *Gluten S*

## ELISA TEST | In vitro analysis

for the quantitative determination of prolamins from wheat (gliadin), rye (secalin) and barley (hordein) in food labeled as gluten-free

ProGnosis Biotech S.A. is ISO 9001:2015 certified by TÜV Hellas (TÜV NORD).

**Use only the current version of Product Data Sheet enclosed with the kit.**

Allergen-Shield Gluten S, A1048/A1096, is an immunoassay method that determines the gliadin and prolamins from wheat, barley and rye content in finished food products labeled as gluten-free. The ELISA kit contains all reagents required for the immunoassay method. The ELISA test is adequate for 96/48 definitions (standards are included). A spectrophotometer for microtiter ELISA plate is required.

**Matrices:**

Bakery products, beverages, breakfast cereal, buckwheat, buckwheat flour, cake mix, cereal, cheese mix,

chocolate cereal, chocolate wafer, cocoa, cocoa cereal, coffee, cooked biscuit, cooked hamburger, corn, corn cereal, crackers, granola bar, ginger dough, ice cream, millet, oat, oat based foodstuff, oat cereal, pasta, quinoa, ready-to-serve meals, rice, rice cereal, sausage sorghum, sorghum flour, soy, soy crisp, soy flour, soup mix, teff, wine

- Sample preparation: extraction and dilution
- Test time (incubation time after samples and reagents preparation): 30min
- Standard curve range: 0 - 80 ppm
- Shelf life: 12 months
- Storage: 2-8°C

## Specifications

- The LOD of the method is 1 ppm gluten or 0.5 ppm gliadin.
- The LOQ of the method is 5 ppm gluten or 2.5 ppm gliadin.
- The recovery<sup>1</sup> of spiked extractions-matrices was 93.9% (CV = 6.9%).
- IC50 = 10 - 30 ppm.
- Each standards duplicates mean CV ≤ 6%.
- Coefficient of Variation (CV) of result at 15 ppm = 5.5% (n=16).
- Coefficient of Variation (CV) of result at 35 ppm = 6.1% (n=16).

No cross-reactivity was observed in a variety of matrices such as: cereals, tree nuts, legumes, seeds, meats and spices. Cross reactivities of the used antibodies have been determined for the pure food (e.g. corn flour). In a composed / processed food (e.g. maize bread) cross reactivities might be different.

- Recovery of gluten spiked matrices was within acceptable AOAC guidelines limits when a large panel of matrices was tested.

## 1. Description

Allergen-Shield Gliadin S is an sandwich enzyme-linked immunosorbent assay (ELISA) test for the detection of gluten in finished food products labeled as gluten-free.

## 2. General Information

Gluten consists of two groups of proteins, namely the glutenins and the prolamins. Prolamins are present in wheat (gliadin), barley (hordein) and rye (secalin), and are the alcohol-soluble fraction of gluten. Consumption of gluten might be harmful for people with gluten intolerance (celiac disease) and wheat allergy, because the small intestine is unable to absorb nutrients. It might cause a broad range of symptoms, such as nausea, vomiting, abdominal pain, joint pain, infertility or frequent miscarriages etc. Moreover, long-term gluten consumption may lead to more severe symptoms. For example, weakening of the bones (osteoporosis) and iron deficiency anemia. According to the Codex Alimentarius (CODEX STAN 118/1979) food labeling is divided into groups, "gluten-free" and "very low gluten" products where the gluten content is lower than 20 mg/kg and 100 mg/kg, respectively.

## 3. Principle of the Method

The presence of gluten in a sample is determined by the immunological detection of gliadin and prolamins. The wells of the microtiter strips are coated with a monoclonal antibody against gliadin. The standard solutions and the solutions of the samples are added and if a specimen contains gliadin, the latter will bind to the immobilized antibody. All of the unbound gliadin will be removed by washing. Then, the detection solution is added (peroxidase-conjugated antibody against gliadin) and binds to gliadin. Any unbound molecule of the detection solution will be removed by washing. A chromogen substrate is then added to the wells resulting in the progressive development of a blue colored complex with the detection antibody. The color development is then stopped by the addition of acid turning the resultant final product yellow. The measurement is made photometrically at 450 nm and the intensity of the produced colored complex is directly proportional to the concentration of gluten present in the samples and the standard solutions.

## 4. Reagents Provided

Allergen-Shield Gluten S ELISA kit contains sufficient reagents and materials for 48/96 measurements (including standard tests).

Reagents (Store at 2-8°C)	Quantity for 48 wells	Quantity for 96 wells	State	Vial cap color
Single-Break Strip Plate	48 wells	96 wells	Ready to use (precoated)	-
Dilution Microwells	48 wells	96 wells	Ready to use (red color)	-
Sealing film	2 sheets	2 sheets	Ready to use	-
Matrix Diluent	1 plastic vial (60ml)	2 plastic vials (each 60ml)	Ready to use	Yellow
Standards 1 - 6 (0, 5, 10, 20, 40 and 80 ppb of Gliadin in aqueous solution) (correspond to 0, 5, 10, 20, 40 and 80 ppm of Gluten)	6 plastic vials (each 1.5ml)	6 plastic vials (each 1.5ml)	Ready to use	Brown
Gluten S Detection Solution	1 plastic vial (8ml)	1 plastic vial (15ml)	Ready to use	Green
Extraction Buffer	1 plastic vial (60ml)	2 plastic vials (each 60ml)	5X Concentrate (dilute in distilled water)	Blue
Wash Buffer	1 plastic vial (50ml)	1 plastic vial (50ml)	20X Concentrate (dilute in distilled water)	White
TMB Substrate	1 plastic vial (8ml)	1 plastic vial (15ml)	Ready to use	Brown
Stop Solution	1 plastic vial (8ml)	1 plastic vial (15ml)	Ready to use	White

## 5. Materials required but not provided

- A grinder sufficient to render sample to particle size of fine instant coffee
- Balance with 0 - 50 g measuring capability and Graduated cylinder - 100mL
- Distilled or deionized water
- Centrifuge, centrifugal vials
- Vortex mixer and/or Shaker
- Microtiter plate reader fitted with 450 nm filter
- Water bath (50 °C / 122 °F)
- 100, 200 and 1000 µL adjustable single channel micropipettes with disposable tips (a repetitive pipette of 100µL is acceptable for the steps of TMB and Stop Solution)
- 50 - 300 µl multi-channel micropipette with disposable tips and reservoirs
- Ethanol or 2-propanol solution 40%
- Skim Milk Powder

## 6. Storage Instructions

Store kit reagents between 2 and 8°C (35 - 46°F). Do not freeze any components provided. Reseal immediately the unused strips of the microtiter plate in the bag together with the desiccant bag provided and store at 2 - 8°C. After use remaining reagents should be returned to cold storage (2 - 8°C). Expiry of the kit and reagents is stated on the labels respectively and no quality guarantee is accepted after the expiration date. The expiry of the kit components can only be guaranteed if the components are stored properly as well as if the reagent is not contaminated by the first handling, in case of repeated use of one component. Because of the colorless TMB Substrate and standards light sensitivity, avoid the exposure to direct light. Do not interchange individual reagents between kits of different lot numbers.

## 7. Safety and Precautions for use

- Ethanol solution is highly flammable. Keep container tightly closed, and keep away from heat, sparks, open flame and those smoking. It is toxic if swallowed, or if vapor is inhaled. **Avoid contact with skin.**
- Avoid any skin contact with standards (Gliadin), Stop Solution (8% H<sub>3</sub>PO<sub>4</sub>) and TMB (toxic). **Use gloves.** In case of contact, wash thoroughly with water.
- All reagents should be warmed in room temperature before use and covered when not in use. **Use a clean disposable plastic pipette tip for each reagent, in order to avoid cross-contamination. When pipetting reagents, maintain a consistent order of addition from well-to-well. This will ensure equal incubation times for all wells.**
- Use a clean plastic container to prepare the wash buffer and all residual washing liquid must be drained from the wells by efficient aspiration or by decantation followed by tapping the plate forcefully on absorbent paper. Never insert the absorbent paper into the well. Read the absorbance within 60 minutes after completion of the assay.

## 8. Indication of corruption of kit reagents

- The bluish coloration of the chromogen substrate before the ELISA test.
- A value of less than 0.7 absorbance units (450nm) for the Standard 1 (S1).

## 9. Reagents and sample preparation

### 9.1 Reagents preparation

- Clean surfaces, glass vials, mincers and other equipment with 40% ethanol or 2-propanol before and after each sample preparation.
- Dilute the 5X extraction solution concentrate 5 fold with distilled water to give a 1X working solution.

**Preparation of Extraction Buffer 1X:** In case of the occurrence of crystals in the Extraction Buffer, the warming by gentle dismantling (using hands) of the crystals is needed. Only the amount which actually is needed should be diluted 1:5 (1+4) with distilled water (e. g. 50 ml concentrate + 200 ml distilled water, sufficient for the extraction of 20 samples). The clean bottle with 1X Extraction Buffer working solution can be left out of the refrigerator during the method procedure and subsequently be stored 2 - 8°C for one month. Make sure that the buffer is not contaminated with gliadin.

- Dilute the 20X wash buffer solution concentrate 20 fold with distilled water to give a 1X working solution.

**Preparation of Wash Buffer 1X:** In case of the occurrence of crystals in the Wash Buffer, the warming by gentle dismantling (using hands) of the crystals is needed. Pour the entire content of the solution concentrate (50ml) into a clean 1000ml graduated cylinder, rinse the vial with distilled or deionized water and pour the content again into the cylinder and fill to a final volume of 1000ml with distilled or deionized water. Mix gently to avoid foaming, transferring the final solution from cylinder to a clean bottle and back two times. The clean bottle with 1X Wash Buffer working solution can be left out of the refrigerator during the method procedure and subsequently be stored 2 - 8°C for one month.

### 9.2 Solid Samples

- The sample must be collected according to established sampling techniques. Grind a representative sample (at least 5 g) to the particle size of fine instant coffee (50% passes through a 20 mesh screen).
- Weigh out a 0.5 g ground portion of the sample, add 10 mL of the Extraction Buffer 1X and incubate for 40 min at 50°C by mixing them periodically on a vortex (e.g. per 15 min). **The ratio of sample to extraction solvent is 1:20 (w/v).**

- Allow the sample to cool down and centrifuge for 10 min, at least 2500 g, at room temperature (20 - 25 °C / 68 - 77 °F) and/or filter the extract (alternatively 2 ml of the extract can be centrifuged with high speed for 10 min in reaction caps by using a microcentrifuge).
- Transfer the supernatant in a screw top vial
- Dilute the sample 1: 25 (40 µL + 960 µL) with matrix diluent. The final dilution factor is **500**.
- Use 150 µL per dilution well in the assay.

**NOTE 1:** The extracted sample should have a pH value of 6.2 - 7.5. If the pH is less than 6.2 as for example happens on the silage samples, the pH should be neutralized using NaOH or HCl.

**NOTE 2:** In case the user makes an additional dilution 1:1 of centrifuged sample with extraction buffer 1X the range of quantification becomes 0 - 160 ppm. So, dilute also 40 µL of each diluted sample with 960 µL matrix diluent and use 150 µL directly in the immunoassay. Multiply the final gluten ppm result x 2.

### 9.3 Liquid Samples

Use 0.5 mL of the sample, add 9.5 mL of the Extraction Buffer 1X and follow the rest of the procedure exactly as in step 9.2.

**NOTE 1:** The centrifuged supernatants can be stored at 4°C for up to one week.

**NOTE 2:** For food matrices containing polyphenols, such as tannins, found in chocolate, fruits, wine, tea, coffee and cocoa, the addition of 5% skim milk powder to the extraction buffer is recommended to achieve optimal results.

## 10. Method Procedure

**10.1 Assay Design:** Determine the number of microwell strips required to test the desired number of samples plus the appropriate number of wells needed for standards. Considering that each sample and standard can be tested in single or in duplicate, create a layout. **NOTE 1:** If the number of wells is more than 32 (four strips), a repetitive pipette or multichannel pipette is necessary. **NOTE 2:** It is recommended to test each sample and standard in duplicate considering Good Laboratory Practices and quality control requirements.

**CAUTION:** Use the standards positions in duplicate as the **Example plate** layout below **NECESSARY** and note positions of samples that can be set to all remaining empty wells of layout in duplicate.

	1	2	3	4	5	6	7	8	9	10	11	12
A	St1	St1										
B	St2	St2										
C	St3	St3										
D	St4	St4										
E	St5	St5										
F	St6	St6										
G												
H												

Example plate layout (example for a 6 point standard curve)

**10.2** Bring all reagents to room temperature (19 - 24°C) before use. Remove the **standards** (1 - 6) and place the **appropriate number** of Dilution Microwells (red) in a microwell holder for each Standard and Sample to be tested. Place an equal number of Antibody Coated Microtiter Wells in another microwell holder. Immediately reseal the unused strips of the microtiter plate in the bag together with the desiccant bag provided. The samples should be stored in a cool place.

**10.3** Using a new pipette tip for each, transfer 150 µL of each standard (Standard 1 - 6) and prepared sample in duplicate (see 10.1) to the red-marked mixing wells.

**10.4** Using a multichannel pipette, transfer 100µl of contents from each Dilution Microwell to a corresponding Antibody Coated Microtiter Well, cover the microwells with the sealing film, shake the microplate manually for 30 seconds and incubate at room temperature for **10 min**.

**10.5** Remove the sealing film and wash the plate as follows: Aspirate the liquid from each well into the sink and tap the holder of microwells upside down strongly (four times in a row) on an absorbent paper to insure the complete removal of liquid from the wells. Dispense **300 µL of Wash Buffer 1X** (see 9.1) into each well with wash bottle or multichannel micropipette using the proper reagent reservoir and shaking the plate manually for a few seconds. Repeat this process for another three times (**total 4 times**). **CAUTION:** It is important to not allow microwells to dry between working steps.

**10.6** Aspirate the liquid as described above and add **100 µL of Gluten S Detection Solution** to each well. If the number of wells is more than 32 (four strips), a repetitive pipette or multichannel pipette is necessary (pour 1 mL of Detection Solution in a reservoir per 8 wells). Cover the microwells with the sealing film, shake the plate manually for a 30 seconds and incubate at room temperature for **10 min**.

**10.7** Remove the sealing film and wash the plate as the wash step 10.5.

**10.8** Aspirate the liquid as described above and add **100 µL** per well of **TMB Substrate** (pour 1mL per 8 wells in a reservoir). Cover the microwells with the sealing film, shaking the plate manually for a few seconds and incubate in the dark at room temperature for **10 min**.

**10.9** Remove the sealing film and add **100 µL** per well of the **Stop Solution** to each well (pour 1 mL per 8 wells in a reservoir). Mix gently by shaking manually.

**10.10** Measure the absorbance at **450 nm**. Read the absorbance value of each well (immediately after the step 10.9 on a spectrophotometer using 450 nm as the primary wavelength and optionally 620 nm as the reference wave length (610 nm to 650 nm is acceptable).

### 11. Data Analysis

#### • Automatically

An assigned software, the **Prognosis-Data-Reader**, is available for free (contact: info@prognosis-biotech.com) download to evaluate the Allergen-Shield Gluten S ELISA kit. The evaluation is carried out by a simple transfer of data values after the measurement.

The gliadin concentration in ng/ml (ppb) is read from the Prognosis-Data-Reader calibration curve. The dilution factor of 500 and the conversion factor of 2 (gliadin represents 50 % of the proteins present in gluten, Codex Definition) in order to convert the gliadin content to gluten content, is already included in the result.


#### • Manually

Calculate the average absorbance values for each set of duplicate standards and samples. Ideally, duplicates should be within 10% of the mean. Use the following calculation:

$$\frac{\text{Standard or sample absorbance}}{\text{Standard 6 absorbance}} \times 100 = \% \text{ Binding}$$

The gluten content in each sample is determined by extrapolating OD values against the gluten content of standard solutions using a fifth order polynomial standard curve. To express results as ppm gliadin, multiply the result by 0.5 (e.g., 5 ppm gluten x 0.5 = 2.5 ppm gluten).

### 12. Example of Standard Curve (0 - 80 ppm)

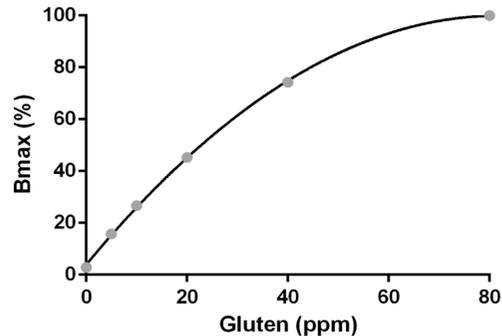

### 13. Performance Evaluation

#### 13.1 Reference Materials

Several reference materials are being used for the evaluation of each product of ProGnosis Biotech S.A. in the context of Quality Control performed by the Quality Control Department. Please request a validation report, including the results, at info@prognosis-biotech.com.

#### 13.2 Proficiency Tests


All products participate frequently in Proficiency Tests. For more information, visit the individual product page on our website: [www.prognosis-biotech.com](http://www.prognosis-biotech.com)

### 14. Assay Claims

- Samples showing negative results may contain Gluten below the limit of detection of the assay. This ELISA kit does not claim that food is safe for consumption based upon a determination of gluten content. Matrix effects may also affect the result of the method.
- The recovery/cross reactivity of the method might be affected when analyzing processed food (e.g. heat treatment, dehydration, etc.), because proteins may be altered or fragmented.
- Food samples that have been heat treated may contain denatured proteins which may not be captured by the antibody. Recovery of these matrices might be reduced.
- A representative sample was used for the cross reactivity evaluation. Other samples may show a different result.
- The protein content and the protein composition may differ among various species of the same matrix. Therefore, different varieties may produce different results.

### 15. Method Summary

Total procedure time (after samples and reagents preparation): 30min

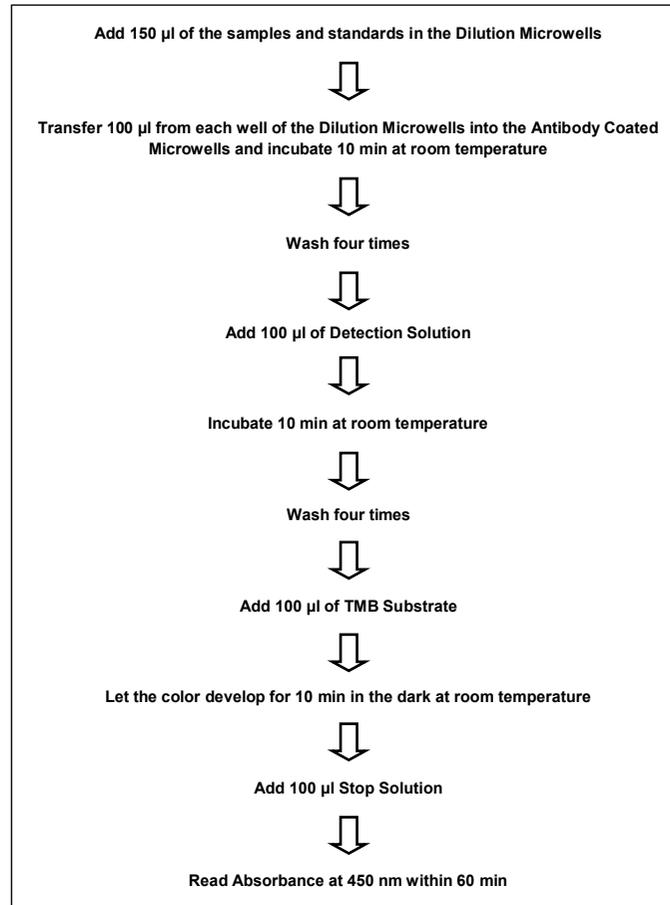

### ELISA TEST | In vitro analysis

for the quantitative determination of prolamins from wheat (gliadin), rye (secalin) and barley (hordein) in food labeled as gluten-free

ProGnosis Biotech S.A. is ISO 9001:2015 certified by TÜV Hellas (TÜV NORD).

**Use only the current version of Product Data Sheet enclosed with the kit.**

Allergen-Shield Gluten S, A1048/A1096, is an immunoassay method that determines the gliadin and prolamins from wheat, barley and rye content in finished food products labeled as gluten-free. The ELISA kit contains all reagents required for the immunoassay method. The ELISA test is adequate for 96/48 definitions (standards are included). A spectrophotometer for microtiter ELISA plate is required.

### Matrices:

Bakery products, beverages, breakfast cereal, buckwheat, buckwheat flour, cake mix, cereal, cheese mix, chocolate cereal, chocolate wafer, cocoa, cocoa cereal, coffee, cooked biscuit, cooked hamburger, corn, corn cereal, crackers, granola bar, ginger dough, ice cream, millet, oat, oat based foodstuff, oat cereal, pasta, quinoa, ready-to-serve meals, rice, rice cereal, sausage sorghum, sorghum flour, soy, soy crisp, soy flour, soup mix, teff, wine

- Sample preparation: extraction and dilution
- Test time (incubation time after samples and reagents preparation): 30min
- Standard curve range: 0 - 80 ppm
- Shelf life: 12 months
- Storage: 2-8°C

All immune assays supplied by ProGnosis Biotech S.A., are warranted to meet or exceed our published specification when used under normal conditions in your laboratory. If the product fails during the stated period, a replacement product will be issued.

ProGnosis Biotech S.A. makes no warranty of any kind, either expressed or implied, except that the materials from which its products are made are of standard quality. There is no warranty of merchantability of this product, or of the fitness of the product for any purpose. ProGnosis Biotech S.A. shall not be liable for any damages, including special or consequential damage, or expense arising directly or indirectly from the use of this product. This method is considered to be a screening method, before a legal action, samples detected as positives must be confirmed with a confirmation method. This product is meant to be used only For Research or Manufacturing use and by qualified technicians.



[www.prognosis-biotech.com](http://www.prognosis-biotech.com)  
 e: info@prognosis-biotech.com  
 t: +30 2410 623922  
 f: +30 700 700 6262  
 Farsalon 153 | 41335 Larissa, Greece

